

TÜV AUSTRIA CERT GMBH
Certification Body



CERTIFICATE OF CONFORMITY


Reg.- No.: TA 380 12 1646


Product:	Infrared Thermometer	Applicant:	GAS DNA CO., LTD. Rm910C, Cdong, Bupyeong Woolim Lion's Valley #425, Cheongcheon-Dong Bupyeong-Gu, Incheon Korea
Type:	IR-80		
Description:			
Certification reference:	EN 61326-1:2018		
Comments:			
Test report:	BWS-12-EC-0022		

The above mentioned product complies with the requirements of the above standards. It fulfills the requirements of Directive 2004/108/EC.

2012-03-18

Date of issue

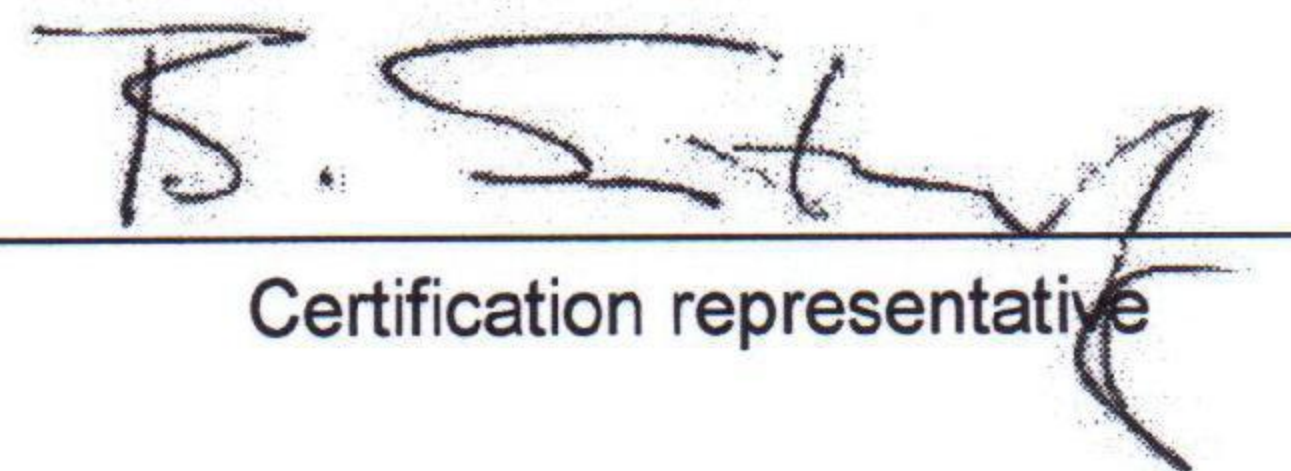
Certification representative

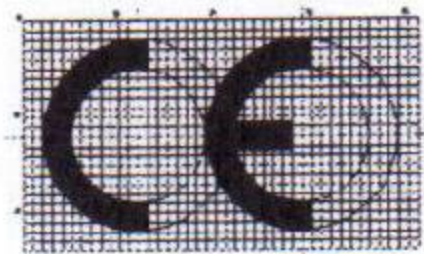

After preparation of the necessary technical documentation as well as the conformity declaration the required CE marking can be affixed on the product. Other relevant directives have to be observed.

„The duplication of this document in parts is subject to the approval by TÜV AUSTRIA CERT GMBH“
The validity of this certificate is notified on the TÜV AUSTRIA Homepage

TÜV AUSTRIA CERT GMBH
A-1015 Wien, Krugerstraße 16
www.tuv.at

Tel.: +43 (0)1 514 07- 6062
Fax: +43 (0)1 514 07- 6065
e-mail: ps@tuv.at

QFM-TAC-ModA-006, Rev.02

ZERTIFIKAT | CERTIFICATE | CERTIFICAT | CERTIFICADO | СЕРТИФИКАТ | شهادة | 证书 | 인증서